



Fortessa_C Sep2018 5B 3R 7V 3UV

Cytometer:	LSRFortessa	User:	Administrator
Cytometer Name:	LSRFortessa-C	Institution:	RPCCC
Serial Number:	R64717700187	Software:	BD FACSDiva 8.0.1
Input Device:	Manual	Date:	9/26/2018 11:15:10 AM
Window Extension:	10.00		


Violet Laser
(405nm)

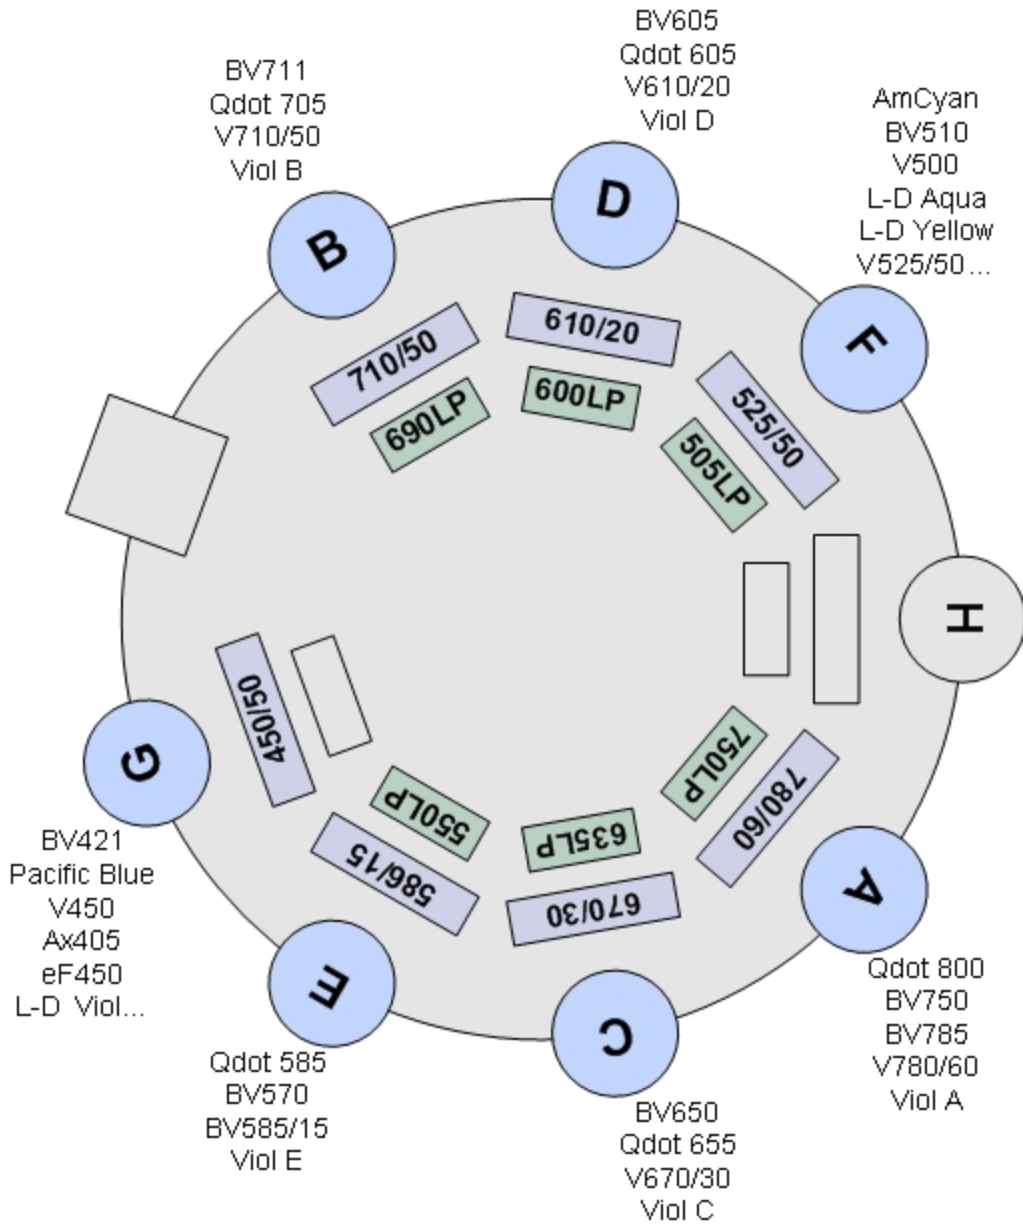


Blue Laser
(488nm)
FSC

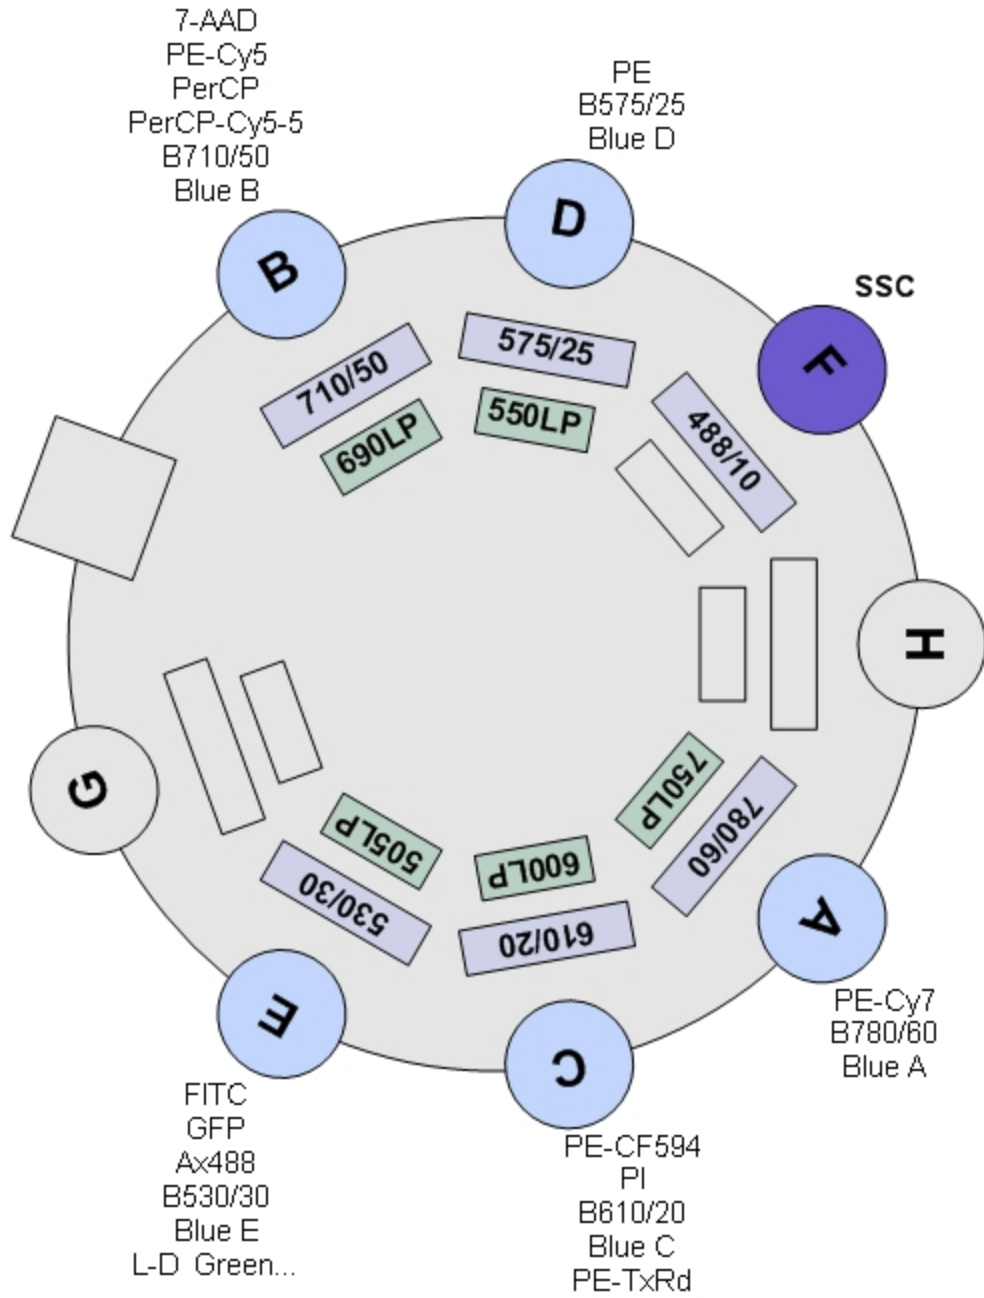

UV Laser
(355nm)

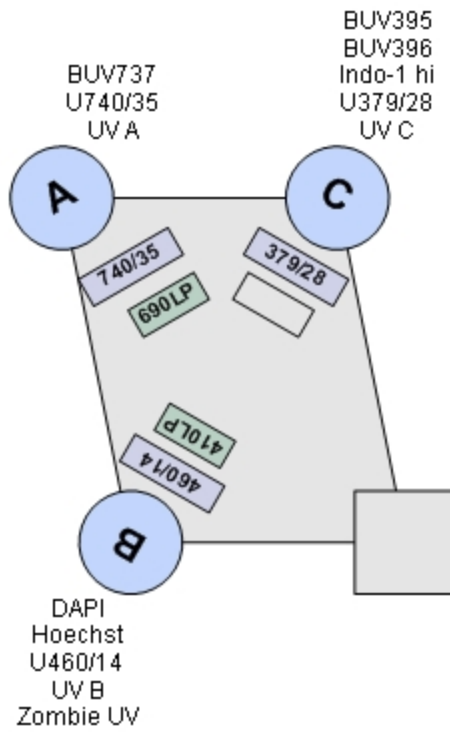

Red Laser
(640nm)

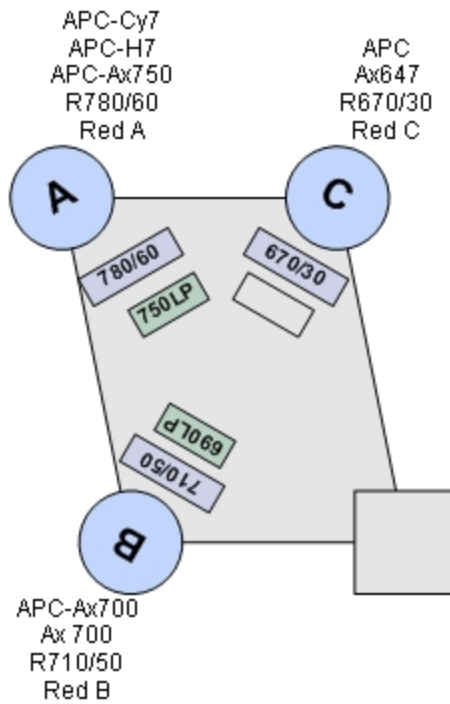

Comments: